

Supporting Information

Simultaneous Multiselective Spectroelectrochemical Fiber-Optic Sensor: Sensing with an Optically Transparent Electrode

Takuya Okazaki,[†] Eri Shiokawa,[†] Tatsuya Orii,[†] Takamichi Yamamoto,[†] Noriko Hata,[†] Akira Taguchi,[‡] Kazuharu Sugawara,[§] and Hideki Kuramitz^{*,†}

[†]Department of Environmental Biology and Chemistry, Graduate School of Science and Engineering for Research, University of Toyama, 3190 Gofuku, Toyama 930-8555, Japan

[‡]Hydrogen Isotope Science Research Center, University of Toyama, 3190 Gofuku, Toyama 930-8555, Japan

[§]Maebashi Institute of Technology, Maebashi, Gunma 371-0816, Japan

Corresponding Author

*E-mail: kuramitz@sci.u-toyama.ac.jp. Tel. & Fax: +81 76 445 6669

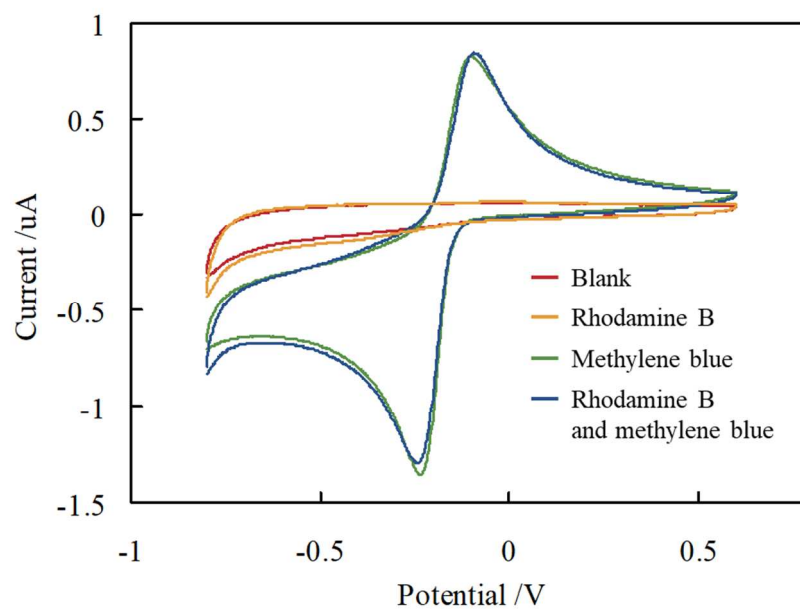


Figure S-1. Cyclic voltammograms of 100 μM rhodamine B, 50 μM methylene blue, and their mixture using a commercial ITO electrode. The measurements were performed at a scan rate of 50 mV/s.