


Supplemental Figure 1A

Silver stained SDS-PAGE gel of fractions used from the 7.5hr rate zonal gradient

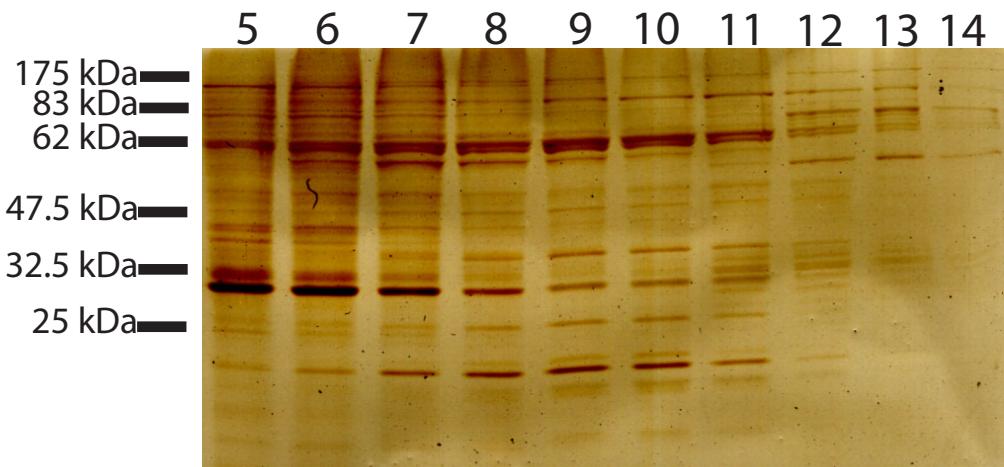

fractions 5, 7, 9, 11 and 13 combined for the pool

Supplemental Figure 1B

Silver stained SDS-PAGE gel of fractions used from the 6.25hr rate zonal gradient

