



J | A | C | S
JOURNAL OF THE AMERICAN CHEMICAL SOCIETY

J. Am. Chem. Soc., 1997, 119(39), 9130-9136, DOI:[10.1021/ja9719945](https://doi.org/10.1021/ja9719945)

Terms & Conditions


Electronic Supporting Information files are available without a subscription to ACS Web Editions. The American Chemical Society holds a copyright ownership interest in any copyrightable Supporting Information. Files available from the ACS website may be downloaded for personal use only. Users are not otherwise permitted to reproduce, republish, redistribute, or sell any Supporting Information from the ACS website, either in whole or in part, in either machine-readable form or any other form without permission from the American Chemical Society. For permission to reproduce, republish and redistribute this material, requesters must process their own requests via the RightsLink permission system. Information about how to use the RightsLink permission system can be found at <http://pubs.acs.org/page/copyright/permissions.html>




ACS Publications

MOST TRUSTED. MOST CITED. MOST READ.

Copyright © 1997 American Chemical Society

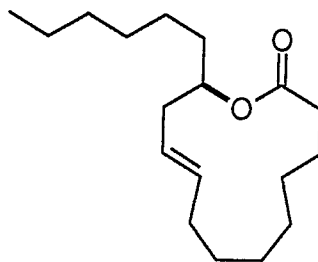

6

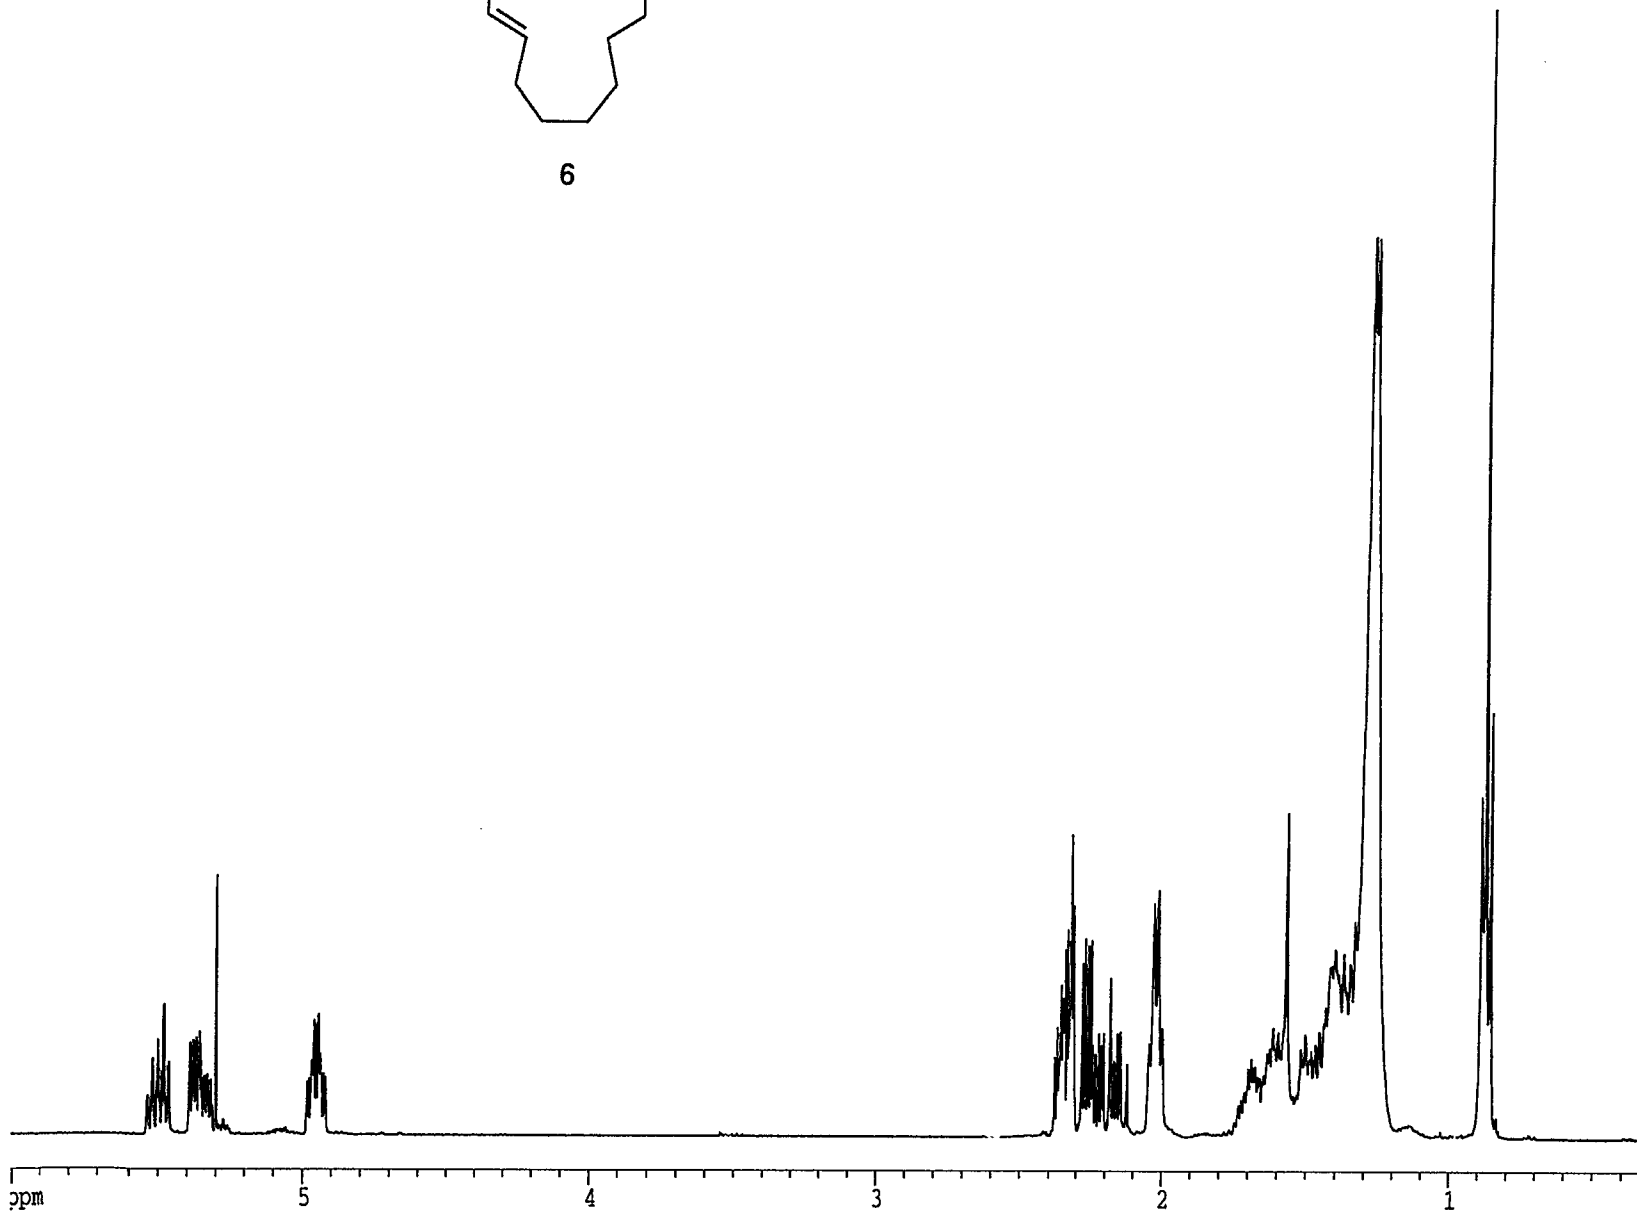

Current Data Parameters
 NAME LGM11804
 EXPNO 10
 PROCNO 1
 DU mpi
 USER kl

F2 - Acquisition Parameters
 Date_ 970411
 Time 14.16
 INSTRUM amx400
 PROBHD 5 mm Multinu
 PULPROG zg30
 TD 32768
 SOLVENT CDCl3
 NS 128
 DS 2
 SWH 8064.474 Hz
 FIDRES 0.246108 Hz
 AQ 2.0316660 sec
 RG 128
 DW 62.000 usec
 DE 88.57 usec
 TE 300.0 K
 HL1 1 dB
 D1 2.00000000 sec
 P1 5.60 usec
 DE 88.57 usec
 SFO1 400.1368403 MHz
 NUCLEUS 1H

F2 - Processing parameters
 SI 32768
 SF 400.1343923 MHz
 WDW no
 SSB 0
 LB 0.00 Hz
 GB 0
 PC 8.00


1D NMR plot parameters
 CX 22.00 cm
 F1P 6.026 ppm
 F1 2411.31 Hz
 F2P 0.322 ppm
 F2 128.73 Hz
 PPMCM 0.25930 ppm/cm
 HZCM 103.75336 Hz/cm

Current Data Parameters
 NAME LGM11804
 EXPNO 10
 PROCNO 1
 DU mpi
 USER kl

F2 - Acquisition Parameters
 Date_ 970411
 Time 14.16
 INSTRUM amx400
 PROBHD 5 mm Multinu
 PULPROG zg30
 TD 32768
 SOLVENT CDCl3
 NS 128
 DS 2
 SWH 8064.474 Hz
 FIDRES 0.246108 Hz
 AQ 2.0316660 sec
 RG 128
 DW 62.000 usec
 DE 88.57 usec
 TE 300.0 K
 HL1 1 dB
 D1 2.00000000 sec
 P1 5.60 usec
 DE 88.57 usec
 SFO1 400.1368403 MHz
 NUCLEUS 1H


F2 - Processing parameters
 SI 32768
 SF 400.1343923 MHz
 WDW no
 SSB 0
 LB 0.00 Hz
 GB 0
 PC 8.00

1D NMR plot parameters
 CX 22.00 cm
 F1P 5.791 ppm
 F1 2317.15 Hz
 F2P 4.629 ppm
 F2 1852.08 Hz
 PPMCM 0.05283 ppm/cm
 HZCM 21.13974 Hz/cm

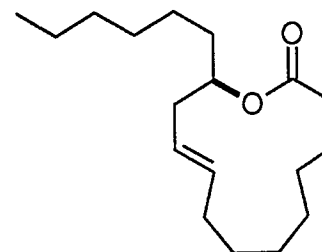

6

E : Z = 98 : 2

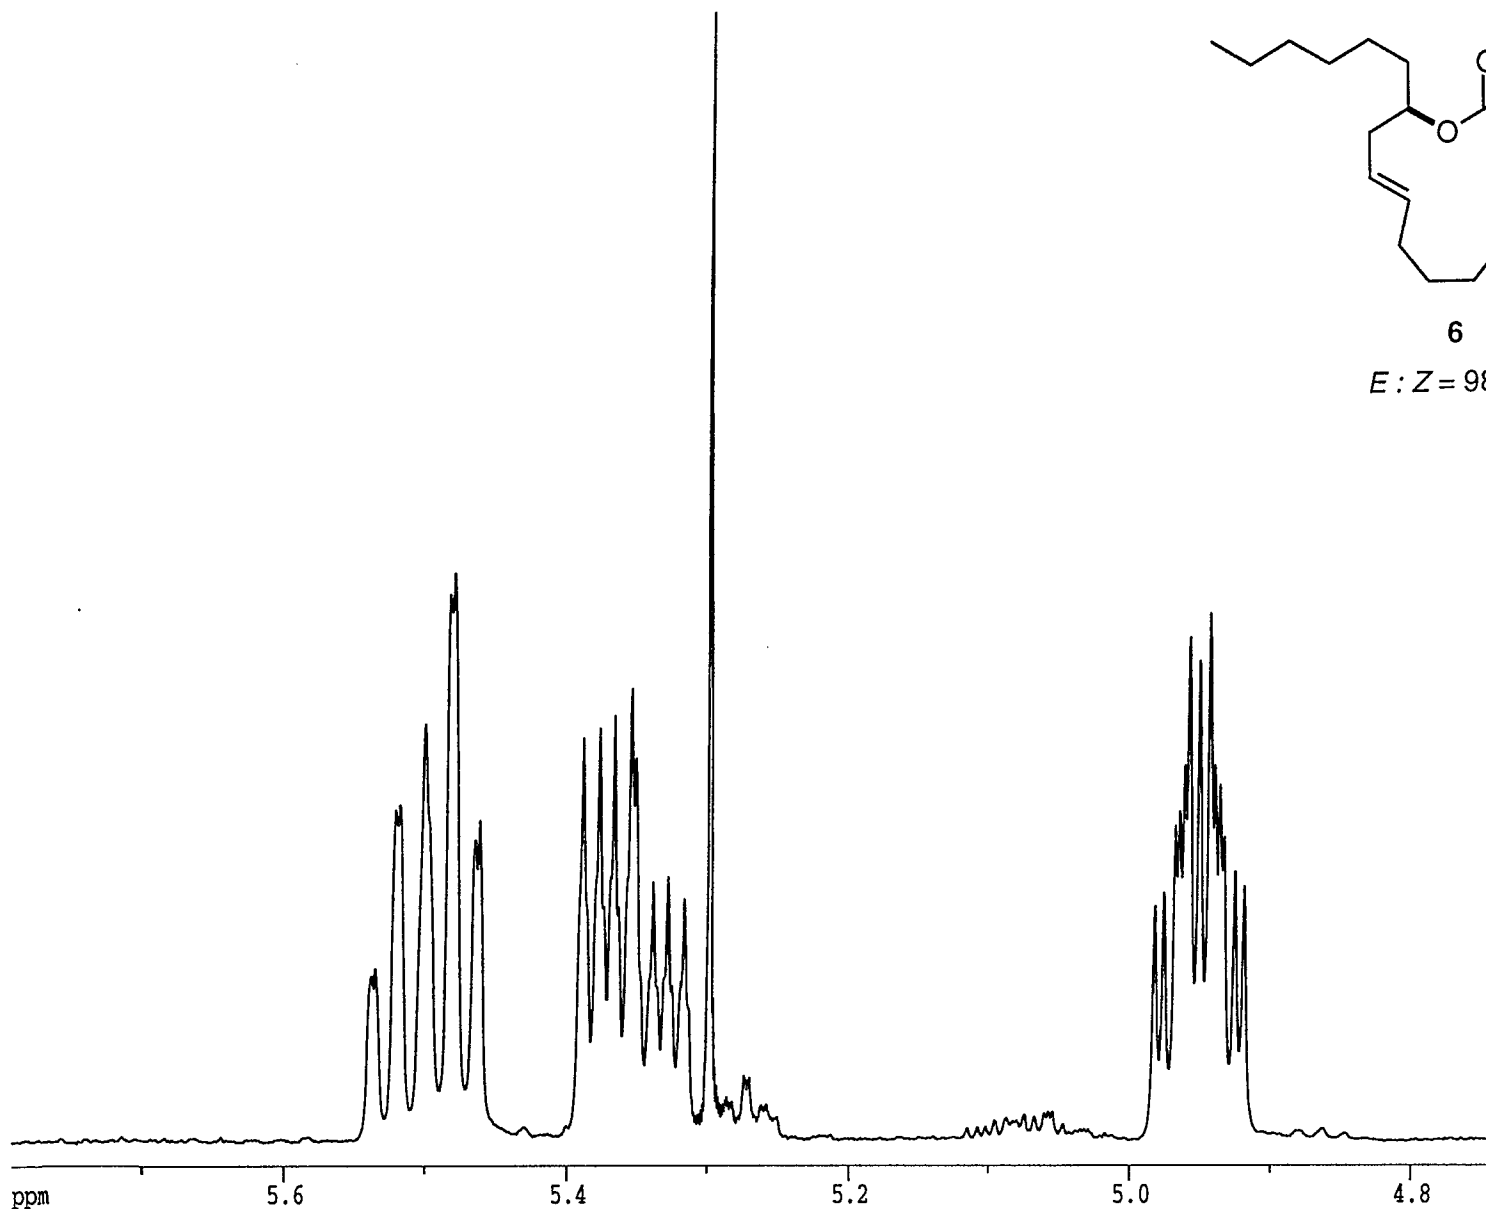


Current Data Parameters
 NAME LGM11804
 EXPNO 10
 PROCNO 1
 DU mpi
 USER kl

F2 - Acquisition Parameters
 Date_ 970411
 Time 14.16
 INSTRUM amx400
 PROBHD 5 mm Multinu
 PULPROG zg30
 TD 32768
 SOLVENT CDCl3
 NS 128
 DS 2
 SWH 8064.474 Hz
 FIDRES 0.246108 Hz
 AQ 2.0316660 sec
 RG 128
 DW 62.000 usec
 DE 88.57 usec
 TE 300.0 K
 HL1 1 dB
 D1 2.00000000 sec
 P1 5.60 usec
 DE 88.57 usec
 SFO1 400.1368403 MHz
 NUCLEUS 1H


F2 - Processing parameters
 SI 32768
 SF 400.1343923 MHz
 WDW no
 SSB 0
 LB 0.00 Hz
 GB 0
 PC 8.00


1D NMR plot parameters
 CX 22.00 cm
 F1P 2.767 ppm
 F1 1107.28 Hz
 F2P 0.601 ppm
 F2 240.35 Hz
 PPMCM 0.09848 ppm/cm
 HZCM 39.40596 Hz/cm

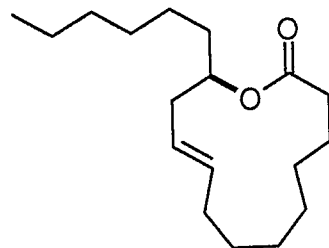

6

E : Z = 98 : 2

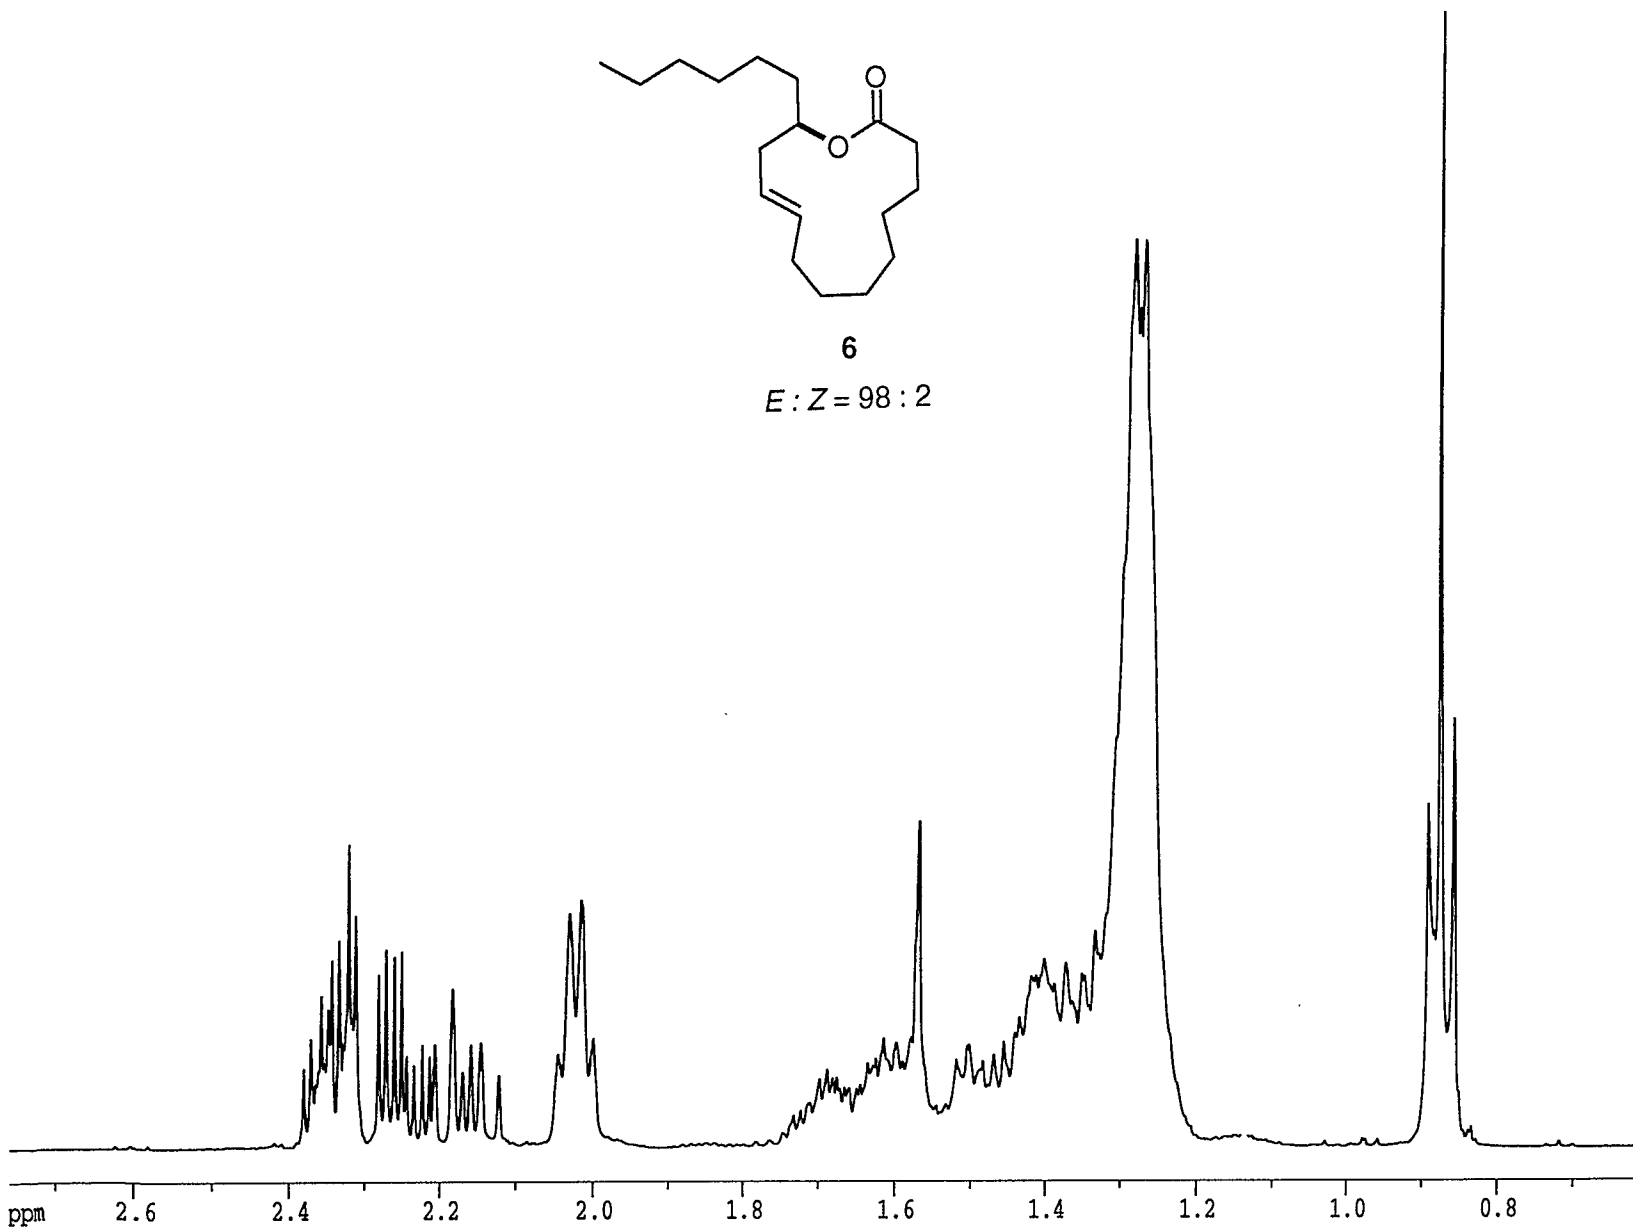

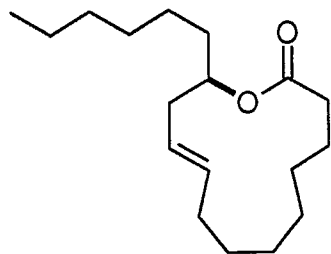

6


E : *Z* = 98 : 2


Current Data Parameters
 NAME LGM11804
 EXPNO 11
 PROCNO 1
 DU mpi
 USER kl

F2 - Acquisition Parameters
 Date_ 970411
 Time 17.02
 INSTRUM amx400
 PROBHD 5 mm Multinu
 PULPROG zgdc30
 TD 65536
 SOLVENT CDCl3
 NS 2958594
 DS 300
 SWH 31249.838 Hz
 FIDRES 0.476835 Hz
 AQ 1.0486259 sec
 RG 32768
 DW 16.000 usec
 DE 22.86 usec
 TE 300.0 K
 D11 0.03000000 sec
 CPDPRG waltz16
 P31 100.00 usec
 S2 28 dB
 HL1 1 dB
 D1 0.01000000 sec
 P1 14.40 usec
 DE 22.86 usec
 SFO1 100.6263997 MHz
 NUCLEUS 13C

F2 - Processing parameters
 SI 65536
 SF 100.6138668 MHz
 WDW no
 SSB 0
 LB 0.00 Hz
 GB 0
 PC 2.00

1D NMR plot parameters
 CX 22.00 cm
 F1P 186.683 ppm
 F1 18782.90 Hz
 F2P -5.884 ppm
 F2 -592.00 Hz
 PPMCM 8.75304 ppm/cm
 HZCM 880.67731 Hz/cm

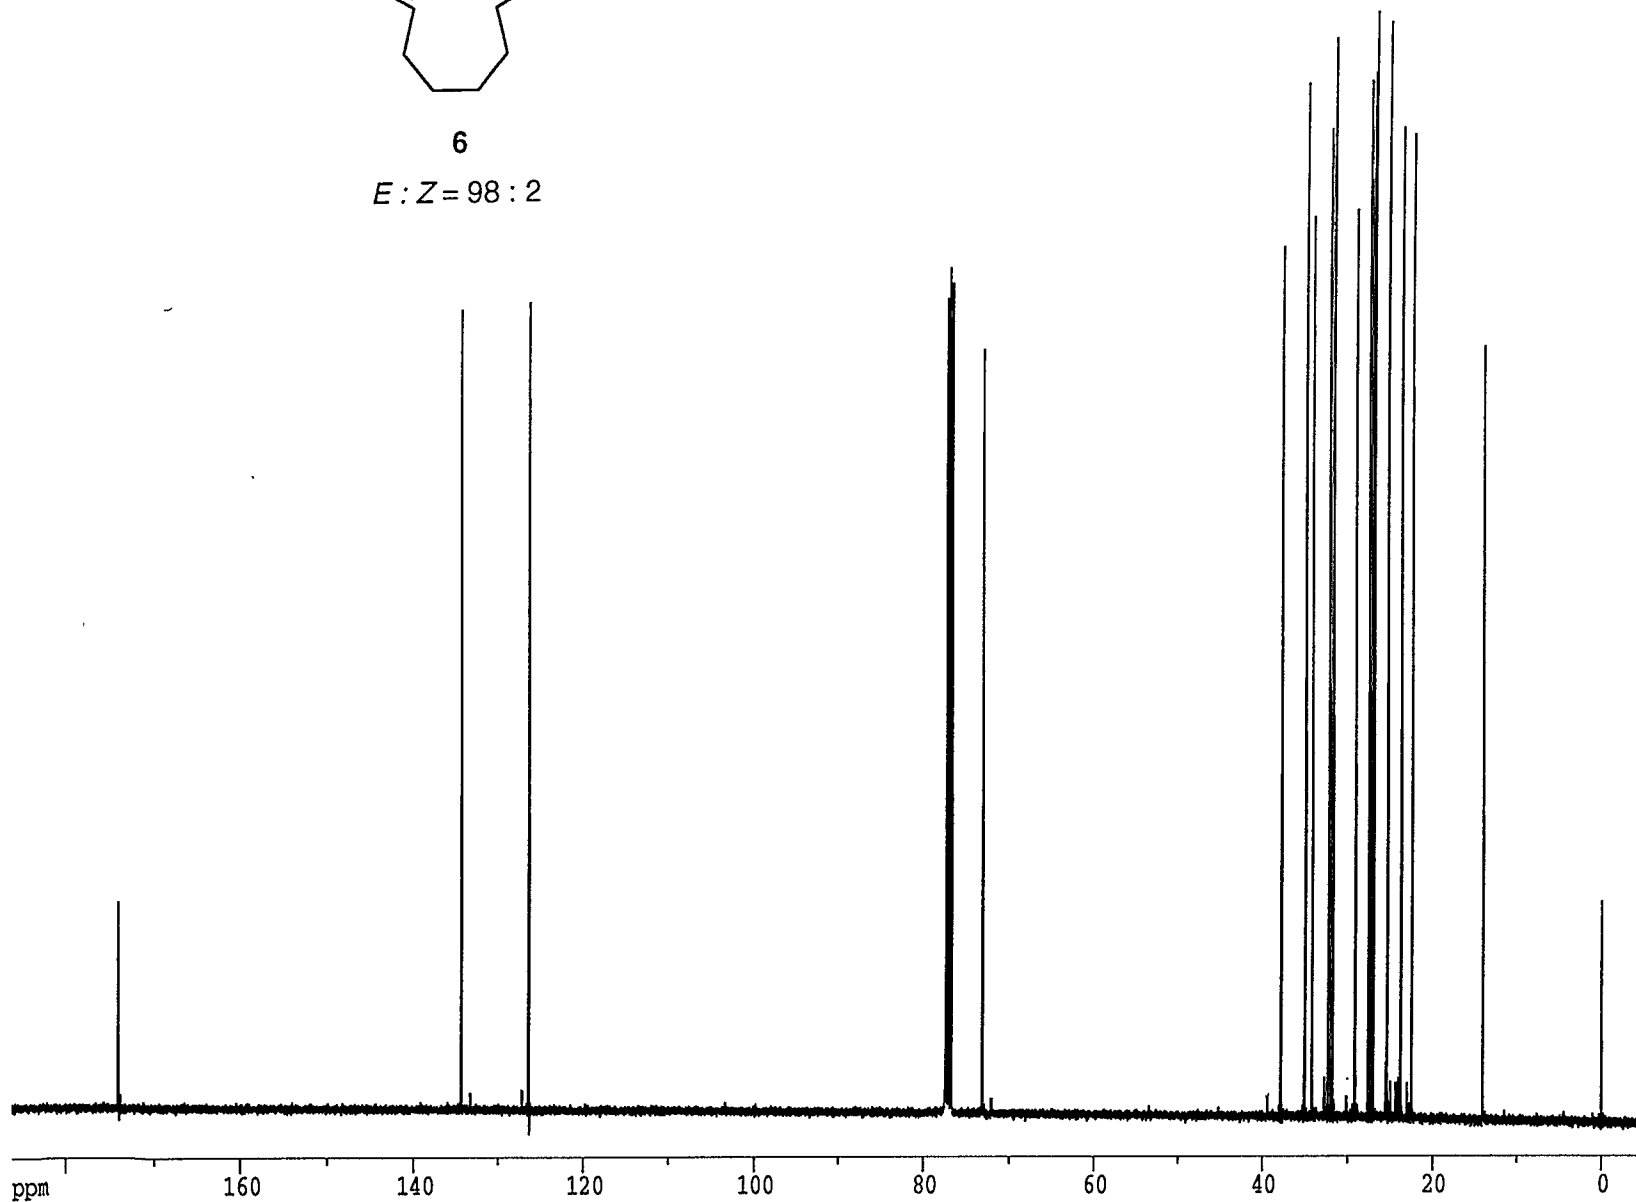

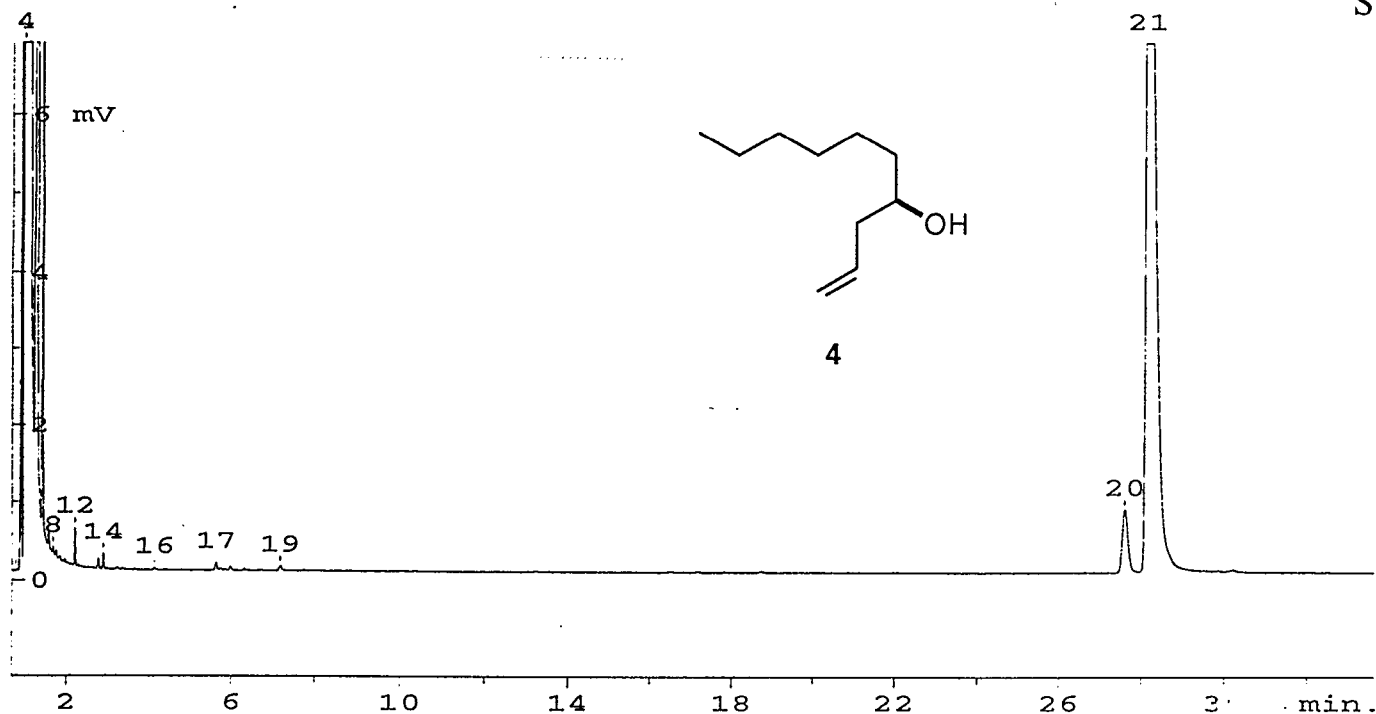

***** r127s100 ***** 22-May-97 16:34:26

Sample : LGM-LB-153-01-97-64619-K measured: 22-May-97 15:46:14
A.-no. : 127 processed: 22-May-97 16:33:57
by: GC
with:

No.	min.	area-%
20	27.61	4.34
21	28.16	95.7

19 peaks had been suppressed.

Instrument : HEWLETT PACKARD 5890
Column : 25MFS/20%TBCD/80%OV1701/N3108 C
Detector : FID
Temperature : 230/80-180/0.8/MIN
Gas : 0.6 BAR H2
Sample size : 0.1
Recorder : 0.2CM/MIN