


RapidFire™ Mass Spectrometry with Enhanced Throughput as an Alternative to Liquid-Liquid Salt Assisted Extraction and LC/MS Analysis for Sulfonamides in Honey


Brian T. Veach, †* Thilak K. Mudalige, † and Peter Rye§

†Office of Regulatory Affairs, Arkansas Regional Laboratory, U.S. Food and Drug Administration, 3900 NCTR Road, Jefferson, Arkansas 72079, United States


§Agilent Technologies, Life Sciences & Diagnostics Group, 121 Hartwell Avenue, Lexington, MA 02421, United States

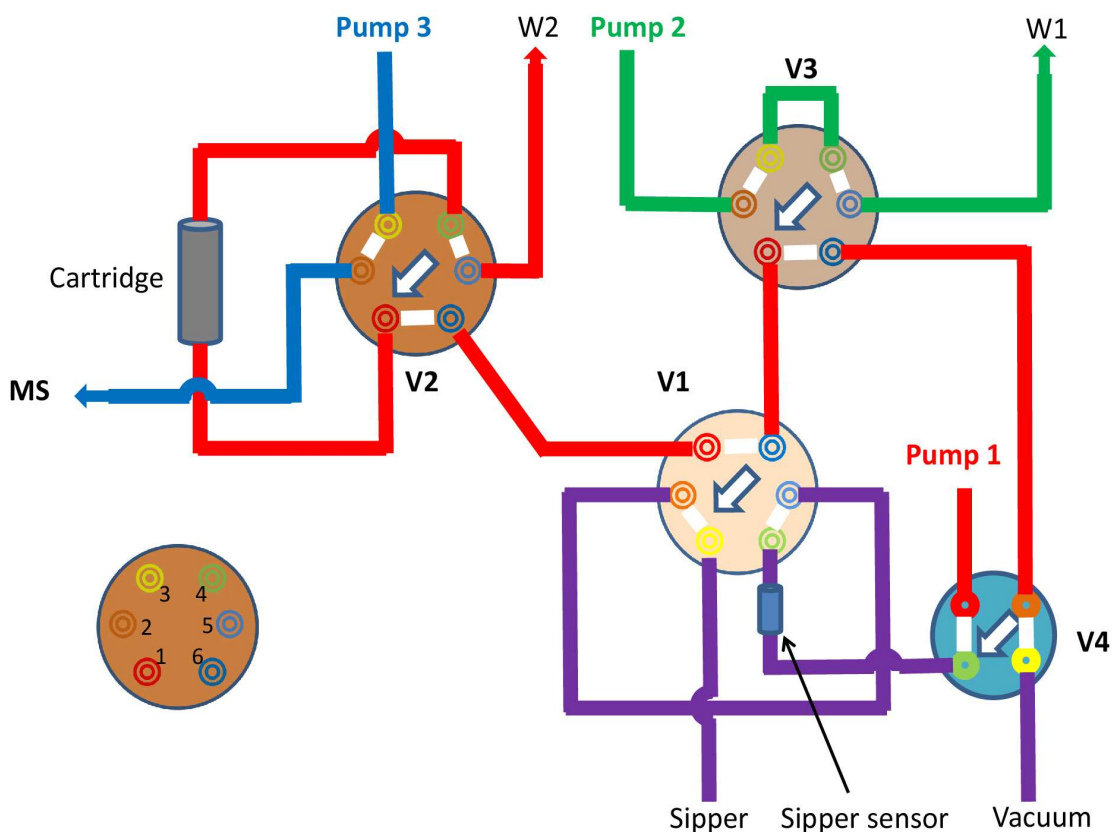


S1. A schematic illustration showing valve configuration and flow path in the aspiration state

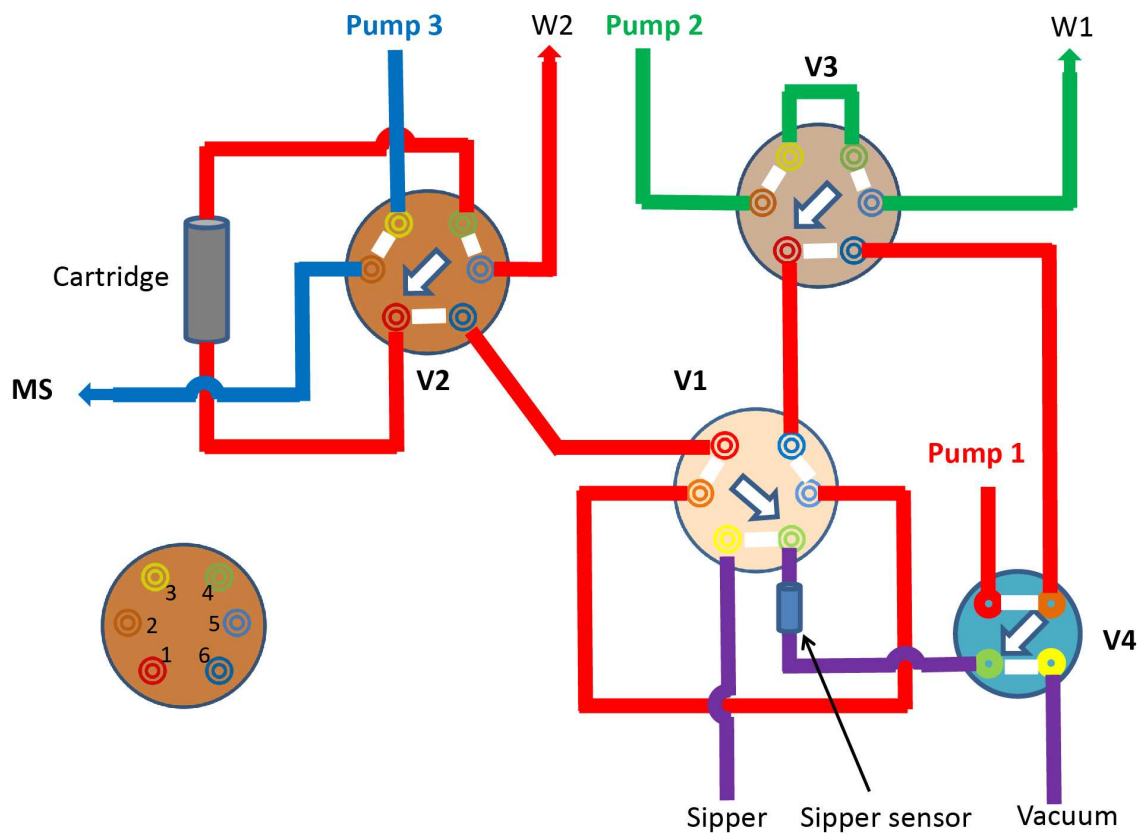


S2. A schematic illustration showing valve configuration and flow path in the load and wash state

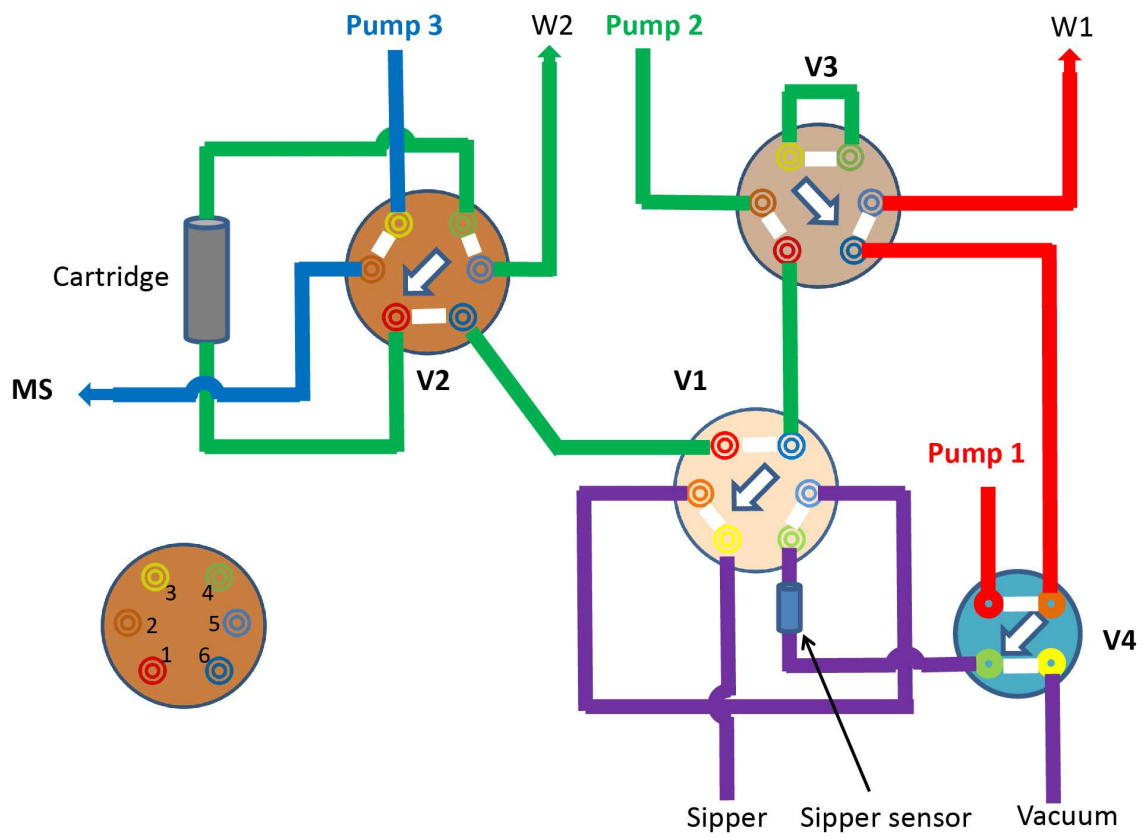

S3. A schematic illustration showing valve configuration and flow path in the extra wash state

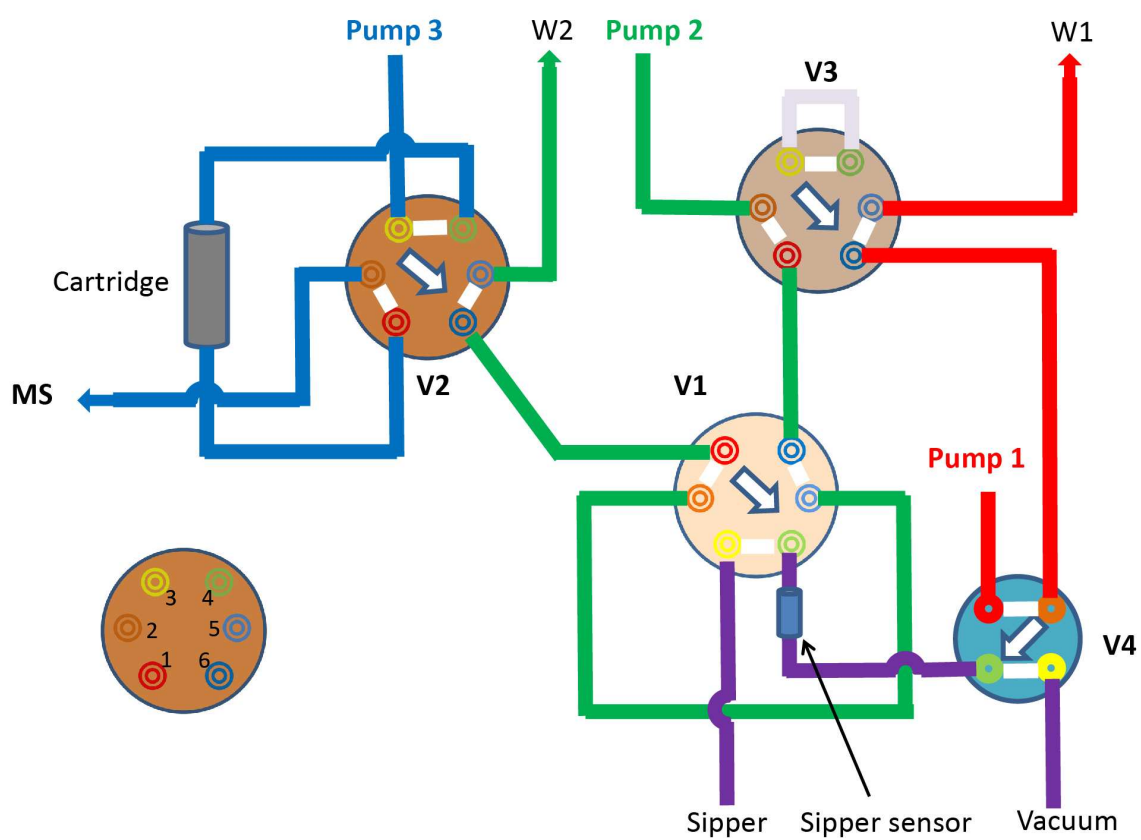

S4. A schematic illustration showing valve configuration and flow path in the elution state

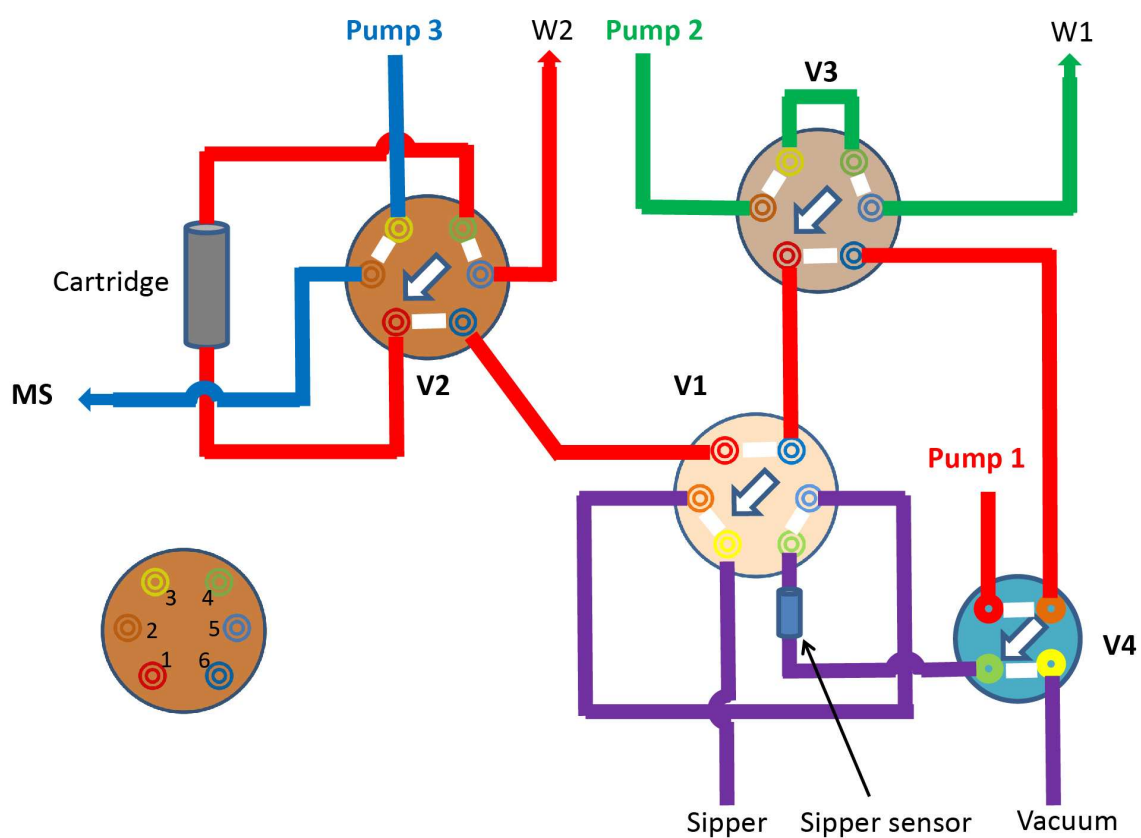

S5. A schematic illustration showing valve configuration and flow path in the re-equilibration state